


Instructions for use:

- * Be sure the regulator is in the "off" position by rotating the knob counterclockwise to the "0" position.
- * For safety, be sure you are not directly in front of or behind the regulator when opening the cylinder valve.
- * SLOWLY turn the cylinder valve on (counterclockwise), about one full turn.
- * If you can hear a hissing sound, there is a leak in the system. Turn the cylinder off and turn the regulator on to relieve any built up pressure. Try tightening the regulator to the cylinder and opening the cylinder again. If this does not help, shut the system down again and contact a service representative. NEVER attempt to repair a regulator or cylinder yourself.
- * Adjust the flow rate setting by turning the knob clockwise until the desired setting shows through the window.
- * If the cylinder pressure falls below 300 PSI, you should exchange the cylinder for a full one.

- * Turn off the system, close the cylinder valve, wait for oxygen to flow out of the regulator, and turn the regulator to the "0" position.
- * NEVER try to remove the regulator unless the cylinder is off and pressure has been relieved.

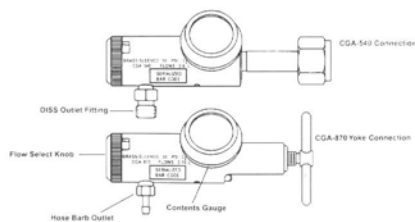

Form#CH-0806 Rev.B

RI

**RESPONSIVE
RESPIRATORY INC.**

261 Wolfner Road
St. Louis, Missouri 63026

Toll Free: 1-866-333-4030
Fax: 1-866-333-4035

Instructions for the operation of Flow Control
Regulators.

Please instruct patient on the enclosed procedures
and provide Him/Her with this manual or a copy
thereof.

OXYGEN FLOW CONTROL REGULATORS

Oxygen flow control regulators are pressure reducing devices which lower oxygen pressure from a cylinder, to levels that can be safely used by the end user.

Oxygen flow control regulators are intended for the administration of oxygen to patients who need increased oxygen levels to improve their breathing conditions. In addition, some models may be used in emergency situations. In an emergency situation, be sure to contact a physician or EMS immediately.

Set-Up (CGA 870 Style)

- * Inspect the cylinder following the instructions of your gas supplier. Be sure to purge the cylinder valve seat of debris.
- * Inspect the regulator for oil or grease. If these are visible, DO NOT use the regulator.
- * Be sure the sealing washer is in place on the inlet to the regulator.
- * Slip the yoke over the cylinder post and fit the pins into the holes on the cylinder valve. The pins should fit easily into these holes.
- * Turn the T-Handle clockwise until the screw point is seated in the dimple on the cylinder valve. Be sure the regulator is tightened securely onto the cylinder.
- * Attach the oxygen supply tubing to the outlet connection of the regulator.

Set-Up (CGA 540 Style)

- * Inspect the cylinder following the instructions of your gas supplier. Be sure to purge the cylinder valve seat of debris.
- * Inspect the regulator for oil or grease. If these are visible, DO NOT use the regulator.
- * Gently thread the large nut on the regulator onto the connection on the the cylinder valve.
- * Tighten the nut with a wrench until snug.
- * Attach the oxygen supply tubing to the outlet connection of the regulator.